

# World Health Products Rating Service

Start from the Bottom and work up  
Click what you can Prove you have

## The QQC Electronic Tongue

11 European Governmental Professional Work Qualifications for using the device. Platinum rating.

10 Taught in accredited medical universities and your device/product appears or your peer reviewed medical studies are quoted in certified medical textbooks. This takes a minimum of seven years in peer reviewed medical journals. Gold rating.

9 Medically supervised, independently researched, double blinds, Peer reviewed medical journal publication Silver Rating.

8 Double Blind Independent Medically Supervised Studies.

7 Independent Medically Supervised Studies.

6 TESTIMONIALS, STORIES OR clinical studies done by your personal staff. Proper Ethics Committees and or Institutional Review Boards are needed, as well as informed consent and full compliance with the Helsinki research accord.

5 SCIENCE + DEVICE STUDIES+ SAFETY Registration+ MEDICAL CLAIM Registration- here your device/product is proven safe, and effective for medical uses in the claims you specify in your registration.

4 SCIENCE + DEVICE STUDIES+ SAFETY Registration- here your device is safety tested to CE standards

3 SCIENCE + DEVICE STUDIES- bench tested for performance specs

2 SCIENTIFIC THEORY- accepted science

1 MAGICAL THINKING SCIENCE- here pseudo-science, unproven theories

0 DIVINATION- the devices subtle muscle control of the therapist


-1 FRAUDULENT-STOLEN – Completely Illegal

whprs

<http://www.worldhealthproductservice.com/index.html>




# QQC™ Electronic Trivector Tongue

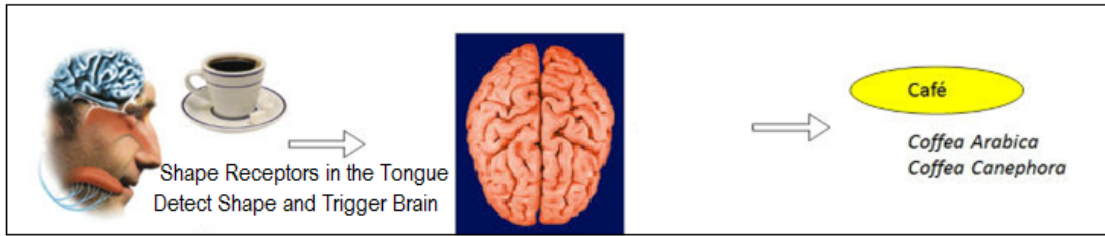

QQC Electronic Tongue Detects the Shape and the SCIO  
Eductor sends the Shape into the Body and the system  
Measures the Electro Physiological Reactivity EPR / TVEP



Café  
*Coffea Arabica*  
*Coffea Canephora*

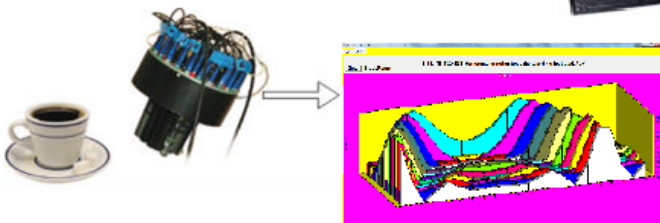


The QQC Trivector Electronic  
Tongue Technology has been  
Reviewed and Published in PEER  
Reviewed Medical Journals and  
printed in Medical University  
Textbooks



Tested, Reviewed, + Recognized  
technology used throughout the  
world today.

## Over 25 yrs Registered Technology

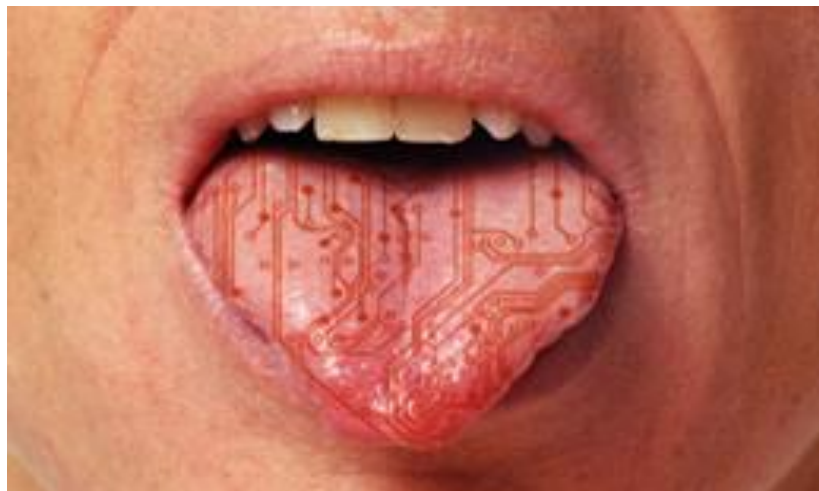

## DECLARATION OF CONFORMITY



**Eclosion kft of Budapest Hungary**

We declare that the device: **QQC Electronic Tongue**

meets all essential requirements for:

### **Class 1 Voltammetry Device**

- Protection of the health and the safety of the user:
  - PN-EN 60950-1:2007
- Electromagnetic compatibility
  - ETSI EN 301 489-1 V1.6.1
  - ETSI EN 301 489-8 V1.2.1
- Effective use of radio frequency spectrum:
  - ETSI EN 301 502 V8.1.2
  - ETSI EN 300 609-4 V8.0.2

**Eclosion Quality Control Officer  
Budapest, Hu Renewed 10-13-2014**